

Accredited for compliance with ISO/IEC 17025-Testing



Accreditation No. 14184.

NorthConnex

NorthConnex

Ambient Air Quality and Weather Monitoring

Validated Report

1st March- 31st March 2020

Report No.: DAT15689

Report issue date: 28th April 2020

Maintenance contract: MC1999

ECOTECH PTY LTD. ABN: 32005752081 1492 Ferntree Gully Rd, Knoxfield VIC. 3180. AUSTRALIA Tel No: 1300 364 946 Fax No: 1300 668 763 Email ecotech@ecotech.com WEB www.ecotech.com

This document shall not be reproduced except for in full, without the written approval of Ecotech Pty Ltd.



NorthConnex

Customer Details		
Customer	Lend Lease Bouygues Joint Venture	
Contact name	Adam Wawrzynak	
Address	55 Coonara Avenue, West Pennant Hills NSW 2125	

Revision History				
Revision	Report ID	Date	Analyst	
0	DAT15689	28/04/2020	Laura Torres	

Report by:

Laura Torres

aura goores

Approved Signatory:

Jon Alexander

Report No: DAT15689

NorthConnex



Table of Contents

Customer Details2
Revision History2
Table of Contents
List of Figures4
List of Tables5
Executive Summary7
1.0 Introduction
2.0 Monitoring and Data Collection
2.1. Siting Details
2.2. Monitored Parameters11
2.3. Data Collection Methods12
2.3.1. Data Acquisition14
2.4. Data Validation and Reporting14
2.4.1. Validation
2.4.2. Validation notes
2.4.3. Reporting15
3.0 Air Quality Standards and Goals16
4.0 Calibrations and Maintenance
4.1. Units and Uncertainties17
4.2. Maintenance
4.2.1. Calibration & Maintenance Summary Tables18
5.0 Results

Report No: DAT15689

NorthConnex



5.1.	Data Capture	25	
5.2.	Air Quality Monthly Summary	27	
5.3.	Graphic Representations	33	
6.0	Valid Data Exception Tables	43	
7.0	Report Summary		
Appendix 1 - Definitions & Abbreviations50			
Appendix 2 - Explanation of Exception Table			

List of Figures

Figure 1: NorthConnex Project Monitoring Station Locations	.9
Figure 2: NorthConnex Project Air Monitoring Stations - CO 8 hours Rolling average graph for March 2020	33
Figure 3: NorthConnex Project Air Monitoring Stations - NO ₂ graph for March 2020	34
Figure 4: NorthConnex Project Air Monitoring Stations - PM ₁₀ 24 Hour graph for March 2020	35
Figure 5: NorthConnex Project Air Monitoring Stations - PM _{2.5} 24 Hour graph March 2020	36
Figure 6: Ashley Avenue – Wind Rose for March 2020	37
Figure 7: Carden Park – Wind Rose for March 2020	38
Figure 8: Headen Park – Wind Rose for March 2020	39
Figure 9: James Park Hornsby – Wind Rose for March 2020	40
Figure 10: Larchmont Place – Wind Rose for March 2020	41
Figure 11: Thornleigh Golf Centre – Wind Rose for March 2020	42

Report No: DAT15689

NorthConnex



List of Tables

Table 1: NorthConnex Project monitoring sites locations 8
Table 2. Monitoring station siting audit against AS/NZS 3580.1.1 2016 10
Table 3. Monitoring station siting audit against AS/NZS 3580.14 2014 10
Table 4: Parameters measured at the NorthConnex Project monitoring stations 11
Table 5: Methods
Table 6: NorthConnex Project - Air Quality Goals
Table 7: Units and Uncertainties
Table 8: NorthConnex Project Ashley Avenue Maintenance Table March 202019
Table 9: NorthConnex Project Carden Park Maintenance Table March 2020
Table 10: NorthConnex Project Headen Park Maintenance Table March 202021
Table 11: NorthConnex Project James Park Hornsby Maintenance Table March 2020 22
Table 12: NorthConnex Project Larchmont Place Maintenance Table March 2020
Table 13: NorthConnex Project Thornleigh Golf Centre Maintenance Table March 2020 24
Table 14: Data Capture for NorthConnex Ambient Air Quality Network 26
Table 15: Percentage of PM _{2.5} Data <026
Table 16: NorthConnex Project Ashley Avenue Exceedences Recorded for March 2020 27
Table 17: NorthConnex Project Carden Park Exceedences Recorded for March 2020 28
Table 18: NorthConnex Project Headen Park Exceedences Recorded for March 2020 29
Table 19: NorthConnex Project James Park Hornsby Exceedences Recorded for March 2020 30
Table 20: NorthConnex Project Larchmont Place Exceedences Recorded for March 202031
Table 21: NorthConnex Project Thornleigh Golf Centre Exceedences Recorded for March 2020
Table 22: Ashley Avenue Valid Data Exception Table 43

Report No: DAT15689

NorthConnex



Table 23: Carden Park Valid Data Exception Table	.44
Table 24: Headen Park Valid Data Exception Table	.45
Table 25: James Park Valid Data Exception Table	.46
Table 26: Larchmont Place Valid Data Exception Table	.47
Table 27: Thornleigh Golf Centre Valid Data Exception Table	.48

Report No: DAT15689

NorthConnex



Executive Summary

NorthConnex is a new multi-lane road link project, joining the M1 Pacific Motorway (formerly known as the F3 Sydney-Newcastle Expressway) at North Wahroonga and the Hills M2 Motorway at Baulkham Hills.

The Project has the following purposes:

- Construction and operation of two road tunnels for traffic traveling north south between the M1 Pacific Motorway and the Hills M2 Motorway.
- M2 integration works.
- Construction of access points and improvements to intersections and interchanges in the vicinity of NorthConnex.
- Construction of ventilation facilities.
- Motorway control Centre.
- 11 temporary construction facilities to support the construction of the proposal.

Ecotech Pty Ltd has been commissioned by Lendlease Bouygues Joint Venture for air quality monitoring, data collection and reporting at six external ambient air quality monitoring stations: Ashley Avenue AQM (Air Quality Monitoring), Carden Park AQM, Headen Park AQM, James Park AQM, Larchmont Place AQM and Thornleigh Golf Centre AQM.

NorthConnex



1.0 Introduction

Ecotech Pty Ltd was commissioned by Lendlease Bouygues Joint Venture to provide monitoring and data reporting for the NorthConnex ambient air quality and weather monitoring network, located as detailed in Table 1. Ecotech commenced data collection in October 2018.

This report presents the available data for March 2020.

The data presented in this report:

- Describes air quality measurements;
- Compares monitoring results;
- Has been quality assured;
- Conforms with NATA accreditation requirements, where applicable.

2.0 Monitoring and Data Collection

2.1. Siting Details

The NorthConnex Project monitoring network consists of six ambient air quality and weather monitoring stations. The stations location and siting details are described below.

Table 1: NorthConnex Project monitoring sites locations

Site Name	Geographical Coordinates	Height Above Sea Level (m)
Ashley Avenue	33°45′13.87″S, 151 °2′45.11″E	126
Carden Park	33°42′48.15″S, 151° 6′33.10″E	187
Headen Park	33°43′29.42″S, 151° 4′ 44.38″E	175
James Park Hornsby	33°42′2.28″S, 151°6′48.59″E	175
Larchmont Place	33°45′24.12″S, 151°2′46.97″E	110
Thornleigh Golf Centre	33°43′28.06″S, 151°5′11.99″E	182





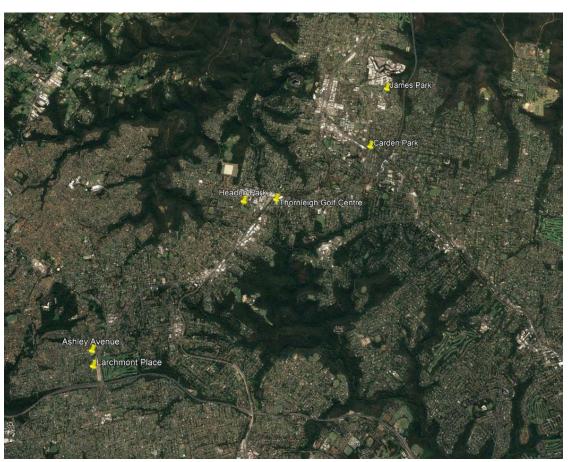


Figure 1: NorthConnex Project Monitoring Station Locations

Stations are audited against the guidelines and mandatory requirements in the standards below, as relevant:

- AS/NZS 3580.1.1:2016 "Methods for sampling and analysis of ambient air guide to siting air monitoring equipment".
- AS/NZS 3580.14:2014 "Methods for sampling and analysis of ambient air Meteorological monitoring for ambient air quality monitoring applications".

Audits against AS/NZS 3580.1.1 2016 were conducted at all sites. Audit results are detailed in Table 2.

NorthConnex



Table 2. Monitoring station siting audit against AS/NZS 3580.1.1 2016

Site Name	Audit date	Site classification	All guidelines met?	Deviations from guidelines
Ashley Avenue	22/11/19	Neighbourhood	Yes	No
Carden Park	17/07/19	Peak	Yes	No
Headen Park	11/02/19	Neighbourhood	Yes	No
James Park Hornsby	18/07/19	Peak	Yes	No
Larchmont Place	3/12/19	Neighbourhood	No	Trees
Thornleigh Golf Centre	4/12/19	Peak	No	Trees

Audits against AS/NZS 3580.14 2014 were conducted at all sites. Audit results are detailed in Table 3.

Table 3. Monitoring station siting audit against AS/NZS 3580.14 2014

Site Name	Audit date	All requirements met	All guidelines met?	Deviations from guidelines
Ashley Avenue	22/11/19	Yes	Yes	No
Carden Park	8/07/19	Yes	Yes	No
Headen Park	1/08/19	Yes	Yes	No
James Park Hornsby	18/07/19	Yes	Yes	No
Larchmont Place	3/12/19	Yes	Yes	No
Thornleigh Golf Centre	4/12/19	Yes	Yes	No

NorthConnex



2.2. Monitored Parameters

Table 4 below details the parameters monitored and the instruments used at the NorthConnex Project monitoring stations. Sampling of all parameters is continuous. For meteorological sensors, the elevation given in the table below is the height above ground level at the monitoring station. For gaseous and particulate parameters, the elevation given in the table below is the sample inlet height above ground level at the monitoring station. Appendix 1 defines any abbreviated parameter names used throughout the report.

Station(s)	Parameter Measured	Instrument and Measurement Technique	Elevation
	СО	Ecotech Serinus 30 – NDIR gas filter correlation infrared photometry	2 m
	NO, NO ₂ , NO _x	Ecotech Serinus 40 – gas phase chemiluminescence	2 m
	PM _{2.5}	Met One BAM 1020 – Beta ray attenuation	2 m
Ashley Avenue Carden Park Headen Park James Park Larchmont Place Thornleigh Golf Centre	PM ₁₀	Thermo – 1405 TEOM (Tapered Element Oscillating Microbalance)	2 m
	Differential Temperature	Met One 062MP	2 m
	Differential Temperature	Met One 062MP	10 m
	Wind Speed (horizontal)	Gill Windsonic Op3	10 m
	Wind Direction	Gill Windsonic Op3	10 m
	Sigma	Calculation	-

Table 4: Parameters measured at the NorthConnex Project monitoring stations

NorthConnex



2.3. Data Collection Methods

Table 5 below shows the methods used for data collection.

Table 5: Methods

Parameter Measured	Data Collection Methods Used	Description of Method	
	AS/NZS 3580.5.1 –1993 ¹	Methods for sampling and analysis of ambient air - Method 5.1: Determination of oxides of nitrogen-Chemiluminescence method	
NO, NO ₂ , NO _x	Ecotech Laboratory Manual	In-house method 6.1 - Oxides of nitrogen by chemiluminescence	
CO	AS/NZS 3580.7.1 –1992 ²	Methods for sampling and analysis of ambient air. Method 7.1: Determination of carbon monoxide—Direct-reading instrumental method	
CO	Ecotech Laboratory Manual	In-house method 6.3 – Carbon monoxide by gas filter correlation spectrophotometry	
PM ₁₀ (TEOM)	AS 3580.9.8-2008	Methods for sampling and analysis of ambient air. Method 9.8: Determination of suspended particulate matter - PM ₁₀ continuous direct mass method using a tapered element oscillating microbalance analyser.	
	Ecotech Laboratory Manual	In-house method 7.3- Particulates - $PM_{2.5}$, PM_{10} by TEOM	
PM _{2.5} (BAM 1020)	AS/NZS 3580.9.12-2013 ³	Methods for sampling and analysis of ambient Air - Method 9.12: Determination of suspended particulate matter—PM _{2.5} beta attenuation monitors	
	Ecotech Laboratory Manual	In-house method 7.5 – Measurement of PM ₁₀ , PM _{2.5} and TSP using Beta Attenuation Monitor	

¹ Superseded by AS 3580.5.1 – 2011 but specifically referenced in ministerial conditions.

² Superseded by AS 3580.7.1 – 2011 but specifically referenced in ministerial conditions.

³ As approved by the Department of Planning and Environment on 8th September 2017.

Report No: DAT15689

NorthConnex



Parameter Measured	Data Collection Methods Used	Description of Method	
Vector Wind Speed	AS 2923-1987 ⁴	Methods for sampling and analysis of ambient air. Method 14: Meteorological monitoring for ambient air quality monitoring applications	
(Horizontal)	Ecotech Laboratory Manual	In-house method 8.1 - Wind speed (Horizontal) by anemometer	
Vector Wind	AS 2923-1987 ⁴	Methods for sampling and analysis of ambient air. Method 14 Meteorological monitoring for ambient air quality monitoring applications	
Direction	Ecotech Laboratory Manual	In-house method 8.3 - Wind direction by anemometer	
Cinus	AS 2923-1987 ⁴	Methods of sampling and analysis of ambient air. Method 14: Meteorological monitoring for ambient air quality monitoring applications	
Sigma	Ecotech Laboratory Manual	In-house method 8.3 Wind direction by anemometer	
Ambient	USEPA (2000) EPA 454/R- 99-005 ⁵	Methods for sampling and analysis of ambient air. Method 14: Meteorological monitoring for ambient air quality monitoring applications	
Temperature	Ecotech Laboratory Manual	In-house method 8.4 – Temperature ambient by thermoelectric techniques	

Note: Two different measurement techniques are used for monitoring PM₁₀ and PM_{2.5} at the NorthConnex Project Stations. Studies conducted in Canada, the United States and other countries have found that the Tapered Element Oscillating Microbalance (TEOM) monitors can under report concentrations compared to the Beta Attenuation Monitors (BAM), especially when the air contains a large proportion of semi-volatile particulate matter, which may be the case during cooler seasons when the air contains less coarse dust and a greater proportion of semi-volatile organic compounds such as those associated with wood smoke. As a result, it is normal

⁴ Superseded by AS/NZS 3580.14 2014 but specifically referenced in ministerial conditions.

⁵ Superseded by AS/NZS 3580.14 2014 but specifically referenced in ministerial conditions.

NorthConnex



to see occasional periods where $PM_{10} < PM_{2.5}$ and this situation does not necessarily indicate a fault with either instrument.

2.3.1. Data Acquisition

Data acquisition is performed using a PC based Congrego logger (using Congrego®) situated at each of the monitoring sites. Each logger is equipped with a 3G modem for remote data collection. The recorded data is remotely collected from the Air Quality Monitoring Station (AQMS) loggers on a daily basis (using Airodis[™] version 5.1.0) and stored at Ecotech's Environmental Reporting Services (ERS) department in Melbourne, Australia. Data samples are logged in 5-minute intervals.

2.4. Data Validation and Reporting

2.4.1. Validation

The Ecotech ERS department performs daily data checks to ensure maximum data capture rates are maintained. Any equipment failures are communicated to the responsible field engineers for urgent rectification. Ecotech ERS maintains two distinct databases containing non-validated and validated data respectively.

The validated database is created by duplicating the non-validated database and then flagging data affected by instrument faults, calibrations and other maintenance activities. The data validation software requires the analyst to supply a valid reason (e.g. backed by maintenance notes, calibration sheets etc.) in the database for flagging any data as invalid.

Details of all invalid or missing data are recorded in the Valid Data Exception Tables.

Validation is performed by the analyst, and the validation is reviewed. Graphs and tables are generated based on the validated five minutes and one-hour data as appropriate.

When considering negative values recorded by the BAM instruments in accordance with the guidelines stated in *AS/NZS 3580.9.12:2013:* "Occasionally BAMs may record short-term (<24 h) negative PM_{2.5} concentrations. This is often associated with the loss of moisture or semi-volatile compounds in the collected particulate matter from the filter media that can occur during the measurement process. Short term negative values resulting from such loss should be considered to be real data and should not be invalidated from the dataset".

NorthConnex



2.4.2. Validation notes

Small daily offset adjustments have been made to correct for zero reference drift in the new CO analysers which should stabilise over time. These adjustments are within the zero tolerances of AS/NZS $3580.7.1 - 1992^5$ and do not impact the data validity.

2.4.3. Reporting

Data is reported in six Microsoft Excel format files named

- NorthConnex_Ashley Avenue_ Monthly Data Report_ March 2020.xls
- NorthConnex_Carden Park_ Monthly Data Report_ March 2020.xls
- NorthConnex_Headen Park_ Monthly Data Report_ March 2020.xls
- NorthConnex_James Park Hornsby_ Monthly Data Report_ March 2020.xls
- NorthConnex_Larchmont Place_ Monthly Data Report_ March 2020.xls
- NorthConnex_ Thornleigh Golf Centre _ Monthly Data Report_ March 2020.xls

Each Excel file consists of 6 worksheets:

- 1. Cover
- 2. Contents
- 3. 5 Minute Data
- 4. 1 Hour Data
- 5. 24-hour Data
- 6. Valid Data Exception Report

The data contained in this report is based on Australian Eastern Standard Time.

All averages are calculated from the five-minute and the one-hour data. Averages are based on a minimum of 75% valid readings within the averaging period. Where data capture is low for a particular parameter, summary values (e.g. monthly maximum and minimum) may be based on less than 75% valid samples. The reader should use caution when interpreting these values as they may not be representative of conditions for the entire sample period.

Averaging periods of eight hours or less are reported for the end of the period, i.e. the hourly average 02:00am is for the data collected from 1:00am to 2:00am. One-hour averages are calculated based on a clock hour. One day averages are calculated based on calendar days.

⁵ Superseded by AS/NZS 3580.7.1 – 2011 but specifically referenced in ministerial conditions.

Report No: DAT15689

NorthConnex



3.0 Air Quality Standards and Goals

The air quality goals and criteria for pollutants monitored at the NorthConnex project ambient monitoring sites are based on SSI 6136 Planning Approval Condition E9. The air quality goals and criteria are shown in Table 6 below.

Note: The measurement uncertainty (as outlined in Table 7) is not considered when assessing exceedences of the air quality standards/goals. Exceedances are only reported for above goal values, based on the decimal places reported. Daily averages for PM_{2.5} are calculated from integer 1 hour measurements and expressed to one decimal place

Table 6: NorthConnex Project - Air Quality Goals

Parameter	Time Period	Goal Level	Units
СО	8 hours (rolling, based on 1-hour averages)	9.0	ppm
NO ₂	1 hour	0.12	ppm
PM ₁₀	1 day	50	µg/m³
PM _{2.5}	1 day	25	μg/m³

Note:

This table includes all valid data points that exceed the defined air quality standards. The Ambient Air Quality NEPM includes a provision for excluding 1-day PM₁₀ or PM_{2.5} averages associated with "exceptional events" from the total exceedences of the Air Quality standard. The definition of an "exceptional event" is included below for reference. It is the responsibility of the end user of this data to evaluate whether any reported exceedences are associated with exceptional events and are eligible to be excluded from the exceedence total. Monitoring and reporting of exceedences during the operational project will be in accordance with the Planning Approval Conditions E7, E8 and E9.

As per the Ambient Air Quality NEPM, *Exceptional event* means a fire or dust occurrence that adversely affects air quality at a particular location, and causes an exceedance of 1 day average standards in excess of normal historical fluctuations and background levels, and is directly related to: bushfire; jurisdiction authorised hazard reduction burning; or continental scale windblown dust.

NorthConnex



4.0 Calibrations and Maintenance

4.1. Units and Uncertainties

The uncertainties for each parameter have been determined by the manufacturer's tolerance limits of the equipment's parameters, and by the data collection standard method.

The reported uncertainties are expanded uncertainties, calculated using coverage factors which give a level of confidence of approximately 95%.

Table 7: Units and Uncertainties

Parameter	Units	Resolution	Uncertainty ⁶	Measurement Range ⁷
NO, NO _x (S40)	ppm	0.001 ppm	± (6% of reading + 0.011 ppm) K factor of 2.0	0 to 0.5 ppm LDL= 0.0004 ppm
NO ₂ (S40)	ppm	0.001 ppm	± (6% of reading + 0.011 ppm) K factor of 2.0	0 to 0.5 ppm LDL= 0.0004 ppm
CO (S30)	ppm	0.1 ppm	0.1 ppm ± (7% of reading + 0.8ppm) K factor of 2.0	
PM _{2.5} (BAM1020)	µg/m³	1 μg/m³	24Hr: ± (5.5 % of reading + 4.0 μg/m ³) (in range 0 - 100 μg/m ³) Hr: ± (8 % of reading + 8.0 μg/m ³ k factor of 2.0	0 to 1000 μg/m ³ LDL _{24hr} =1.0 μg/m ³ LDL _{hr} =4.8 μg/m ³
PM ₁₀ (TEOM)	µg/m³	0.1 μg/m³	$\pm 5.0~\mu g/m^3$ or 3.6% of reading, whichever is the greater K factor of 2.0	0 μg/m ³ to 1 g/m ³ LDL=5μg/m ³
Vector Wind Speed	m/s	0.1 m/s	±0.4 m/s or 2 % of reading, whichever is greater K factor of 2.0	0 to 30 m/s
Vector Wind Direction	deg	1 deg	±4 deg K factor of 2.0	0 to 360 deg Starting threshold: 0 m/s

⁶ Uncertainties are calculated based on the full measurement range unless stated otherwise

⁷ The max measurement range for gas analysers is defined as the full scale (FS=Span/0.8)

Report No: DAT15689

NorthConnex



Parameter	Units	Resolution	Uncertainty ⁶	Measurement Range ⁷
Ambient Temperature	К	0.1 К	± 0.6 K K factor of 2.0	263.15 to 323.15 K

4.2. Maintenance

4.2.1. Calibration & Maintenance Summary Tables

The last calibrations for the following parameters were performed on the indicated dates. Data supplied after this time is subject to further validation, to be performed at the next calibration cycle.

Note: Maintenance and calibration dates may differ, as calibrations may be less frequent than scheduled maintenance visits.

Table 8-13 indicate when the particulate and gas and meteorological equipment were last maintained/calibrated.

"Calibration cycle" refers to the frequency of calibrations and intermediate calibration checks. The most frequent check or calibration is listed here.

NorthConnex



Table 8: NorthConnex Project Ashley Avenue Maintenance Table March 2020

Parameter	Date of Last Maintenance	Maintenance Type	Date of Last Calibration	Prior Calibration	Calibration Cycle
NO, NO ₂ , NO _x	25/03/2020	3-monthly	25/03/2020	17/02/2020	Monthly
со	25/03/2020	Monthly	25/03/2020	17/02/2020	Monthly
PM ₁₀	25/03/2020	3-monthly	25/03/2020	4/12/2019	3-monthly
PM _{2.5}	25/03/2020	Monthly	17/02/2020	4/12/2019	3-monthly
WS/WD/Sigma	25/03/2020	3-monthly	28/06/2018	28/06/2018	2-yearly
Differential Temperature 2m	25/03/2020	3-monthly	4/12/2019	9/08/2019	Yearly
Differential Temperature 10m	25/03/2020	3-monthly	4/12/2019	9/08/2019	Yearly

NorthConnex



Table 9: NorthConnex Project Carden Park Maintenance Table March 2020

Parameter	Date of Last Maintenance	Maintenance Type	Date of Last Calibration	Prior Calibration	Calibration Cycle
NO, NO ₂ , NO _x	25/03/2020	3-monthly	25/03/2020	10/02/2020	Monthly
СО	25/03/2020	Monthly	25/03/2020	10/02/2020	Monthly
PM ₁₀	25/03/2020	3-monthly	25/03/2020	3/12/2019	3-monthly
PM _{2.5}	25/03/2020	Monthly	10/02/2020	3/12/2019	3-monthly
WS/WD/Sigma	25/03/2020	3-monthly	26/06/2018	26/06/2018	2-yearly
Differential Temperature 2m	25/03/2020	3-monthly	5/12/2019	19/08/2019	Yearly
Differential Temperature 10m	25/03/2020	3-monthly	5/12/2019	19/08/2019	Yearly

NorthConnex



Table 10: NorthConnex Project Headen Park Maintenance Table March 2020

Parameter	Date of Last Maintenance	Maintenance Type	Date of Last Calibration	Prior Calibration	Calibration Cycle
NO, NO ₂ , NO _x	4/03/2020	3-monthly	4/03/2020	12/02/2020	Monthly
СО	4/03/2020	Monthly	4/03/2020	12/02/2020	Monthly
PM ₁₀	4/03/2020	3-monthly	4/03/2020	2/12/2019	3-monthly
PM _{2.5}	4/03/2020	Monthly	12/02/2020	2/12/2019	3-monthly
WS/WD/Sigma	4/03/2020	3-monthly	27/06/2018	27/06/2018	2-yearly
Differential Temperature 2m	4/03/2020	3-monthly	2/12/2019	1/08/2019	Yearly
Differential Temperature 10m	4/03/2020	3-monthly	2/12/2019	1/08/2019	Yearly

NorthConnex



Table 11: NorthConnex Project James Park Hornsby Maintenance Table March 2020

Parameter	Date of Last Maintenance	Maintenance Type	Date of Last Calibration	Prior Calibration	Calibration Cycle
NO, NO ₂ , NO _x	25/03/20	3-monthly	25/03/20	4/02/2020	Monthly
СО	25/03/20	Monthly	25/03/20	5/02/2020	Monthly
PM ₁₀	25/03/20	3-monthly	25/03/20	4/12/2019	3-monthly
PM _{2.5}	25/03/20	Monthly	4/02/2020	4/12/2019	3-monthly
WS/WD/Sigma	25/03/20	3-monthly	26/06/2018	26/06/2018	2-yearly
Differential Temperature 2m	25/03/20	3-monthly	5/12/2019	19/08/2019	Yearly
Differential Temperature 10m	25/03/20	3-monthly	5/12/2019	19/08/2019	Yearly

NorthConnex



Table 12: NorthConnex Project Larchmont Place Maintenance Table March 2020

Parameter	Date of Last Maintenance	Maintenance Type	Date of Last Calibration	Prior Calibration	Calibration Cycle
NO, NO2, NOx	30/03/2020	3-monthly	30/03/2020	17/02/2020	Monthly
СО	30/03/2020	Monthly	30/03/2020	17/02/2020	Monthly
PM ₁₀	30/03/2020	3-monthly	30/03/2020	3/12/2019	3-monthly
PM _{2.5}	30/03/2020	Monthly	17/02/2020	3/12/2019	3-monthly
WS/WD/Sigma	30/03/2020	3-monthly	27/06/2018	27/06/2018	2-yearly
Differential Temperature 2m	30/03/2020	3-monthly	3/12/2019	9/08/2019	Yearly
Differential Temperature 10m	30/03/2020	3-monthly	3/12/2019	9/08/2019	Yearly

NorthConnex



Table 13: NorthConnex Project Thornleigh Golf Centre Maintenance Table March 2020

Parameter	Date of Last Maintenance	Maintenance Type	Date of Last Calibration	Prior Calibration	Calibration Cycle
NO, NO ₂ , NO _x	27/03/2020	Non-scheduled	27/03/2020	4/03/2020	Monthly
СО	4/03/2020	Monthly	4/03/2020	3/01/2020	Monthly
PM ₁₀	4/03/2020	3-monthly	4/03/2020	3/12/2019	3-monthly
PM _{2.5}	4/03/2020	Monthly	3/01/2020	3/12/2019	3-monthly
WS/WD/Sigma	4/03/2020	3-monthly	28/06/2018	28/06/2018	2-yearly
Differential Temperature 2m	4/03/2020	3-monthly	4/12/2019	1/08/2019	Yearly
Differential Temperature 10m	4/03/2020	3-monthly	4/12/2019	1/08/2019	Yearly

NorthConnex



5.0 Results

5.1. Data Capture

Valid data capture refers to the amount of valid data collected during the report period. It is based on 5-minute data, for gaseous and meteorological parameters and 1-hour data for particulate parameters.

The percentage of valid data captured is calculated using the following equation:

Valid Data capture = (Reported air quality data / Total data) x 100%

Where:

- Reported air quality data = Number of samples (instrument readings) which have been validated through a quality assured process and excludes all data errors, zero data collection due to calibration, equipment failures, planned and unplanned maintenance.
- Total data = Total number of samples (instrument readings) expected for the sampling period. Total data is calculated based on the same averaging period as "reported air quality data" and the duration of the corresponding report period. e.g. for 5-minute data collected over a month of 31 days, the total data would be equal to 12 (5-minute samples in an hour) x 24 (hours in a day) x 31 (days in a month) = 8928 samples.

Table 14 below displays data capture statistics for March 2020. **Bold** values in the table indicate data capture below 95%.

Table 15 below displays the percentage of negative values in the valid PM_{2.5} data provided.

Details of all invalid or missing data affecting data capture are included in the Valid Data Exception Tables, see section 6.0/ attached Excel file.

NorthConnex



Table 14: Data Capture for NorthConnex Ambient Air Quality Network

	Data Capture (%)							
Parameter	Ashley Avenue	Carden Park	Headen Park	James Park	Larchmont Place	Thornleigh Golf Centre		
PM _{2.5}	99.7	99.7	99.5	99.7	99.7	99.9		
PM ₁₀	85.1	99.8	99.7	99.8	98.3	99.7		
СО	95.8	95.7	95.7	95.8	93.7	95.8		
NO, NO ₂ , NO _x	96.4	96.3	96.2	96.3	96.1	95.0		
WS, WD, Sigma	99.9	99.9	99.9	100.0	100.0	100.0		
AT 2m	0.0	99.9	99.9	100.0	100.0	100.0		
AT 10m	100.0	99.9	99.9	100.0	100.0	100.0		

Table 15: Percentage of PM_{2.5} Data <0

Percentage of PM _{2.5} Data <0 (%)							
AshleyCardenHeadenJamesLarchmontThornleAvenueParkParkParkPlaceGolf Cer							
3.6	3.6	11.5	15.1	5.7	1.6		

NorthConnex



5.2. Air Quality Monthly Summary

Table 16-21 below include a summary of any exceedances recorded at the NorthConnex Project stations during the reported period⁸.

Table 16: NorthConnex Project Ashley Avenue Exceedences Recorded for March 2020

Parameter	Time Period	Value of Exceedence	Date of Exceedence
NO ₂ (ppm)	1 hour	-	-
CO (ppm)	8-hour rolling	-	-
PM ₁₀ (μg/m ³)	24 hour	-	-
PM _{2.5} (μg/m³)	24 hour	-	-

 $^{^{8}}$ Exceedances are reported for above goal values, based on the decimal places reported. Daily averages for PM_{2.5} are calculated from integer 1-hour measurements and expressed to one decimal place.



NorthConnex

Table 17: NorthConnex Project Carden Park Exceedences Recorded for March 2020

Parameter	Time Period	Value of Exceedence	Date of Exceedence
NO ₂ (ppm)	1 hour	-	-
CO (ppm)	8-hour rolling	-	-
PM ₁₀ (μg/m ³)	24 hour	-	-
PM _{2.5} (μg/m³)	24 hour	-	-



NorthConnex

Table 18: NorthConnex Project Headen Park Exceedences Recorded for March 2020

Parameter	Time Period	Value of Exceedence	Date of Exceedence
NO ₂ (ppm)	1 hour	-	-
CO (ppm)	8-hour rolling	-	-
PM ₁₀ (μg/m ³)	24 hour	-	-
PM _{2.5} (μg/m³)	24 hour	-	-

NorthConnex



Table 19: NorthConnex Project James Park Hornsby Exceedences Recorded for March2020

Parameter	Time Period	Value of Exceedence	Date of Exceedence
NO ₂ (ppm)	1 hour	-	-
CO (ppm)	8-hour rolling	-	-
PM ₁₀ (μg/m³)	24 hour	-	-
PM _{2.5} (µg/m³)	24 hour	-	-



NorthConnex

Table 20: NorthConnex Project Larchmont Place Exceedences Recorded for March 2020

Parameter	Time Period	Value of Exceedence	Date of Exceedence
NO ₂ (ppm)	1 hour	-	-
CO (ppm)	8-hour rolling	-	-
PM ₁₀ (μg/m ³)	24 hour	-	-
PM _{2.5} (μg/m³)	24 hour	-	-





Table 21: NorthConnex Project Thornleigh Golf Centre Exceedences Recorded for March2020

Parameter	Time Period	Value of Exceedence	Date of Exceedence
NO ₂ (ppm)	1 hour	-	-
CO (ppm)	8-hour rolling	-	-
PM ₁₀ (μg/m³)	24 hour	-	-
PM _{2.5} (μg/m³)	24 hour	-	-





5.3. Graphic Representations

This section displays graphs of the pollutants and meteorological parameters monitored at the NorthConnex sites for March 2020. The graphs are based on validated 5 minutes or 1-hour data as applicable.

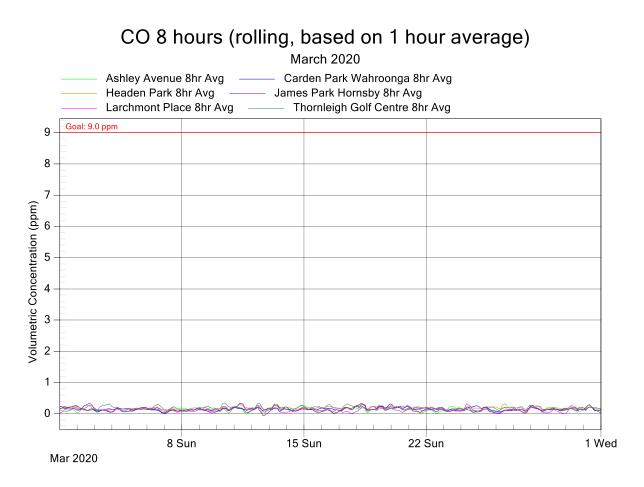


Figure 2: NorthConnex Project Air Monitoring Stations - CO 8 hours Rolling average graph for March 2020

NorthConnex



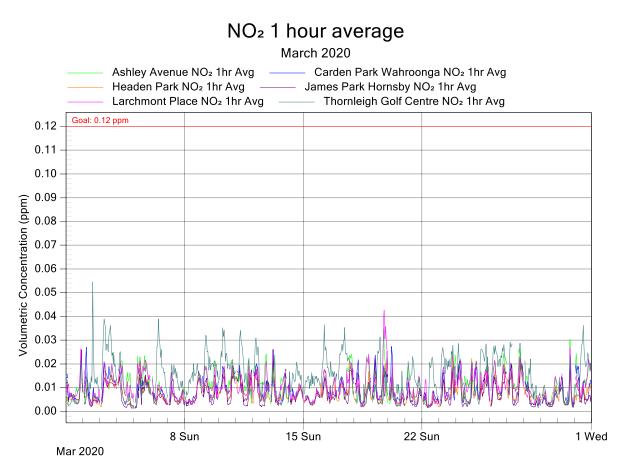


Figure 3: NorthConnex Project Air Monitoring Stations - NO₂ graph for March 2020

NorthConnex



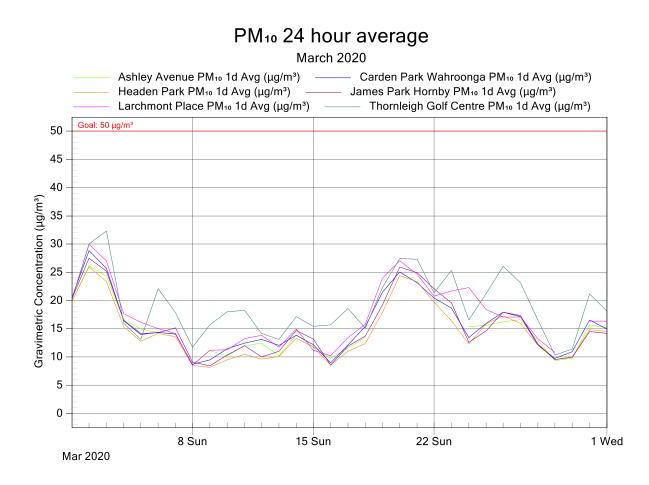


Figure 4: NorthConnex Project Air Monitoring Stations - PM₁₀ 24 Hour graph for March 2020

NorthConnex



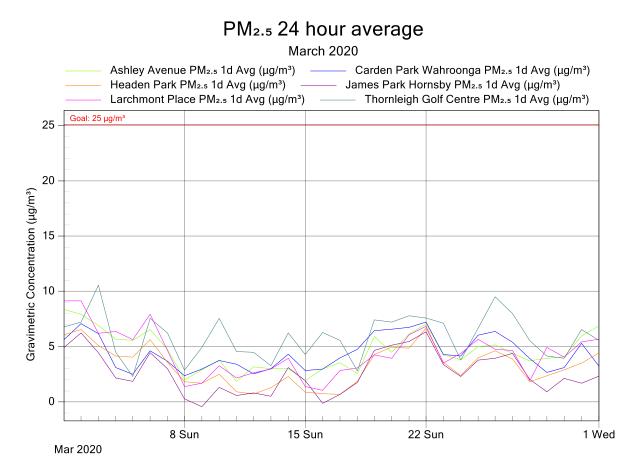


Figure 5: NorthConnex Project Air Monitoring Stations - PM_{2.5} 24 Hour graph March 2020

NorthConnex




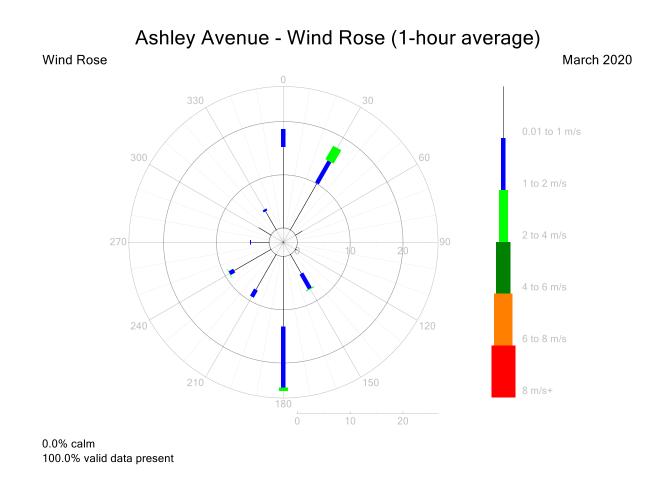


Figure 6: Ashley Avenue – Wind Rose for March 2020

NorthConnex



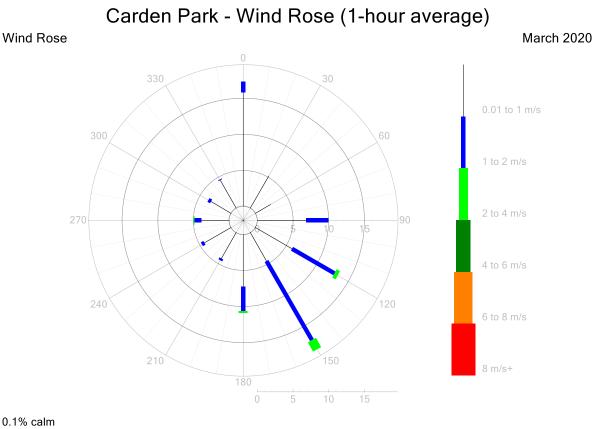


100.0% valid data present

Figure 7: Carden Park – Wind Rose for March 2020

NorthConnex



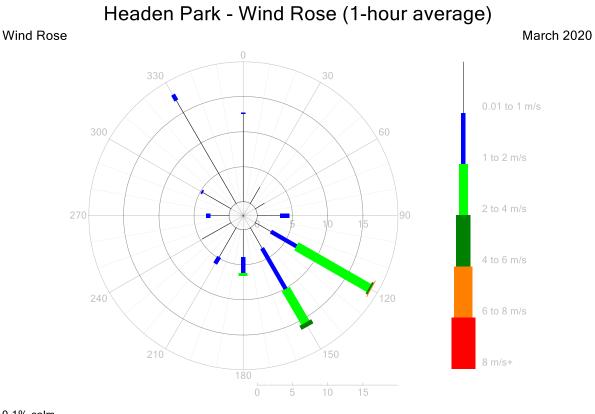


0.1% calm 99.9% valid data present

Figure 8: Headen Park – Wind Rose for March 2020

NorthConnex



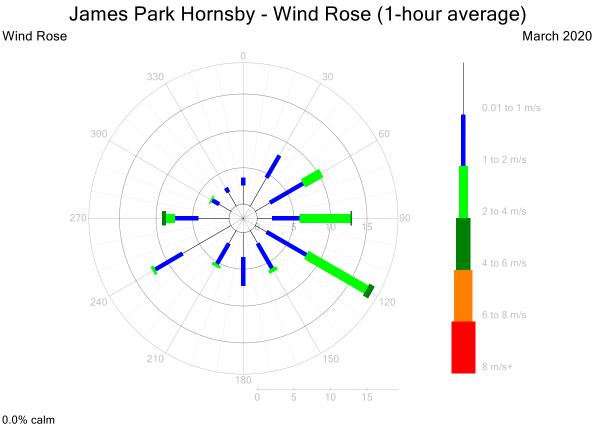


100.0% valid data present

Figure 9: James Park Hornsby – Wind Rose for March 2020

NorthConnex



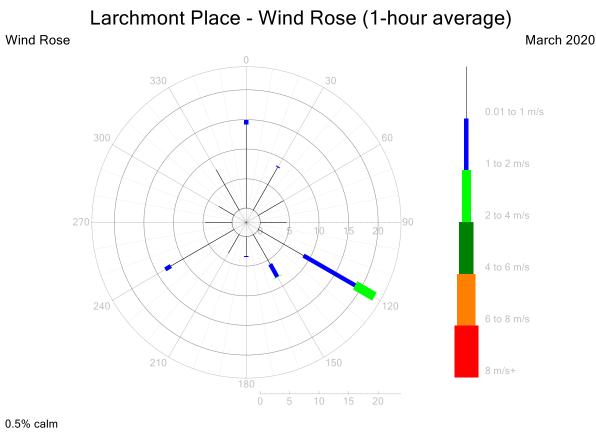


100.0% valid data present

Figure 10: Larchmont Place – Wind Rose for March 2020

NorthConnex



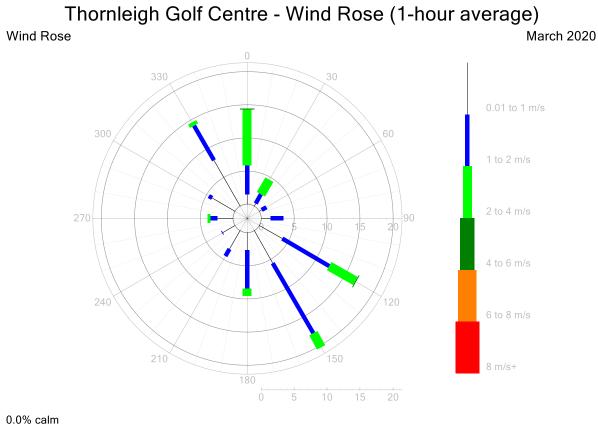

100.0% valid data present

Figure 11: Thornleigh Golf Centre – Wind Rose for March 2020

NorthConnex



6.0 Valid Data Exception Tables

Table 22-27 below detail all changes made to the raw data set during the validation process. An explanation of reasons given in the table can be found in Appendix 2.

Table 22: Ashley Avenue Valid Data Exception Table

Start Date	End Date	Reason	Change Details	User Name	Change Date
01/03/20 00:00	01/04/20 00:00	Instrument fault AT2m		LT	17/04/2020
01/03/20 01:00	31/03/20 01:45	Automatic span and zero checks once daily for 50 minutes CO, NO, NO ₂ , NO _x		LT	17/04/2020
01/03/20 01:50	31/03/20 23:40	Uinear offset applied as required to correct daily baseline drift after overnight span CO A values range are 0.00 ppm and B values range from -0.35 to 0.30 ppm	LT	17/04/2020	
01/03/20 17:30	01/03/20 17:40	Additional background check and subsequent instrument stabilisation		LT	17/04/2020
01/03/20 23:45	31/03/20 23:50	Background checks once daily for 5 - 15 minutes		LT	17/04/2020
19/03/20 15:30	24/03/20 02:15	No data	PM10	LT	17/04/2020
24/03/20 02:15	24/03/20 03:50	Power failure and subsequent instrument stabilisation	CO, NO, NO ₂ , NO _x , PM ₁₀ , PM _{2.5}	LT	17/04/2020
25/03/20 14:20	25/03/20 16:55	Scheduled 3-monthly maintenance	CO, NO, NO ₂ , NO _x , PM ₁₀ , PM _{2.5}	LT	17/04/2020
25/03/20 15:40	25/03/20 23:40	O Static offset of 0.10 ppm applied to correct baseline CO LT		LT	17/04/2020

NorthConnex



Table 23: Carden Park Valid Data Exception Table

Start Date	End Date	Reason	Change Details	User Name	Change Date
01/03/20 01:00	31/03/20 01:45	Automatic span and zero checks once daily for 50-60 minutes	CO, NO, NO ₂ , NO _x	LT	17/04/2020
01/03/20 23:45	31/03/20 23:45	Background checks once daily for 5 - 10 minutes	со	LT	17/04/2020
14/03/20 07:55	31/03/20 08:30	Intermittent data transmission errors	CO, NO, NO ₂ , NO _x , AT2m, AT10m, WS, WD, Sigma, PM ₁₀	LT	17/04/2020
17/03/20 06:00	17/03/20 06:35	Power failure	All parameters	LT	17/04/2020
18/03/20 10:40	18/03/20 10:40	Unrealistic negative data	NO, NO ₂ , NO _x	LT	17/04/2020
25/03/20 10:55	25/03/20 12:00	Scheduled 3-monthly maintenance	CO, NO, NO ₂ , NO _x , PM ₁₀ , PM _{2.5}	LT	17/04/2020

NorthConnex



Table 24: Headen Park Valid Data Exception Table

Start Date	End Date	Reason	Change Details	User Name	Change Date
01/03/20 00:00	01/04/20 00:00	1 ppm and -0.10 ppm applied as (0)		20/04/2020	
01/03/20 05:00	31/03/20 05:45	Automatic span and zero checks once daily for 45 to 50 minutes	CO, NO, NO ₂ , NO _x	LT	20/04/2020
01/03/20 23:45	31/03/20 23:45	Background checks once daily for 5 - 10 minutes	со	LT	20/04/2020
02/03/20 05:50	02/03/20 06:50	Additional instrument stabilisation after span and zero checks	со	LT	20/04/2020
04/03/20 09:00	04/03/20 12:20	Scheduled 3-monthly maintenance	All parameters	LT	20/04/2020
05/03/20 05:50	06/03/20 23:40	Linear offset of A= -0.20 ppm and B= 0.00 ppm applied to correct baseline drift after overnight span	со	LT	20/04/2020
13/03/20 06:45	13/03/20 06:45	Unrealistic negative data	NO, NO ₂ , NO _x	LT	20/04/2020

NorthConnex

WORLD RECOGNISED ACCREDITATION

Table 25: James Park Valid Data Exception Table

Start Date	End Date	Reason	Change Details	User Name	Change Date
01/03/20 01:00	31/03/20 01:45	Automatic span and zero checks once daily for 45 - 55 minutes		LT	20/04/2020
01/03/20 01:50	29/03/20 23:00	Linear offset applied as required to correct daily baseline drift after overnight span A values are 0.00 ppm and B values range from -0.10 to 0.20 ppm	со	LT	20/04/2020
01/03/20 23:05	31/03/20 23:05	Background checks once daily for 5 - 10 minutes	со	LT	20/04/2020
11/03/20 18:25	13/03/20 14:20	Intermittent data transmission errors	CO, NO, NO ₂ , NO _x , AT2m, AT10m, WS, WD, Sigma, PM_{10}	LT	20/04/2020
25/03/20 08:15	25/03/20 11:00	Scheduled 3-monthly maintenance	CO, NO, NO ₂ , NO _x , PM ₁₀ , PM _{2.5}	LT	20/04/2020

NorthConnex



Table 26: Larchmont Place Valid Data Exception Table

Start Date	End Date	Reason	Change Details	User Name	Change Date
01/03/20 01:00	31/03/20 01:45	Automatic span and zero checks once daily for 50 minutes		LT	21/04/2020
01/03/20 01:50	25/03/20 23:40	Linear offset applied as required to correct daily baseline drift after overnight span A values are 0.00 ppm and B values range from 0.10 to 0.25 ppm	ct daily overnight CO LT 2 om and B		21/04/2020
01/03/20 23:45	31/03/20 23:50	Background checks once daily for 5 - 15 minutes	со	LT	21/04/2020
07/03/20 08:50	31/03/20 19:05	Intermittent additional background checks	со	LT	21/04/2020
20/03/20 01:50	27/03/20 23:40	Static offset ranges from -0.30 ppm to 0.10 ppm applied as required to correct the baseline		LT	21/04/2020
24/03/20 02:00	24/03/20 03:55	Power failure followed by instrument stabilisationCO, NO, NO2, NO PM10, PM2.5		LT	21/04/2020
30/03/20 08:05	30/03/20 13:15	Scheduled 3-monthly CO, NO, NO ₂ , NO _x , maintenance PM ₁₀		LT	21/04/2020
30/03/20 13:20	30/03/20 20:40	Additional instrument PM10 LT		LT	21/04/2020
31/03/20 01:50	31/03/20 15:05	Instrument fault CO L		LT	21/04/2020
31/03/20 03:00	31/03/20 03:00	Instrument fault - beta count alarm	PM _{2.5}	LT	21/04/2020
31/03/20 15:10	31/03/20 15:20	Non-scheduled maintenance - connected remotely and reset unit	со	LT	21/04/2020

NorthConnex



Start Date	End Date	Reason	Change Details	User Name	Change Date
01/03/20 01:00	31/03/20 01:45	Automatic span and zero checks once daily for 45-50 minutes	CO, NO, NO ₂ , NO _x	LT	21/04/2020
01/03/20 07:10	30/03/20 04:40	Intermittent unrealistic negative data	NO, NO2, NOx	LT	21/04/2020
01/03/20 23:40	31/03/20 23:45	Background checks once daily for 5 - 10 minutes	со	LT	21/04/2020
04/03/20 08:15	04/03/20 12:30	Scheduled 3-monthly maintenance	All parameters	LT	21/04/2020
24/03/20 01:50	27/03/20 09:30	Linear multiplier of A= 1.04 and B= 1.07 applied to correct span out of tolerance	NO, NO2, NOx	LT	21/04/2020
27/03/20 09:35	27/03/20 16:50	Non-scheduled maintenance - remotely ran NO _x calibration	NO, NO2, NOx	LT	21/04/2020



NorthConnex



7.0 Report Summary

- Percentage availability for most parameters at NorthConnex Project was above 95%, except:
 - PM₁₀ and AT2m at Ashley Avenue
 - CO at Larchmont Place

Refer to Table 14 and Table 22-27 for details.

- There were no exceedances of the air quality goals at the NorthConnex Ambient Air Quality Monitoring Network for the reporting month. Please refer to Table 14-19 in Section 5.2 Air Quality Monthly Summary for further information.
- It is noted that the percentage of negative PM_{2.5} readings recorded for James Park and Headen Park was 15.1% and 11.5% respectively. This will be further investigated in consultation with the independent auditor. Refer to table 15 for further details.
- Travel restrictions in place due to the Covid-19 pandemic have significantly reduced general road traffic which may have had a positive impact on general air quality in the area.

NorthConnex



Appendix 1 - Definitions & Abbreviations

ERS	Environmental Reporting Services
AQMS	Air Quality Monitoring Station
AQM	Air Quality Monitor
BAM	Beta Attenuation Monitors
TEOM	Tapered Element Oscillating Microbalance
0	Degrees (True North)
К	Kelvin
LDL	Lower detectable limit
µg/m³	Micrograms per cubic metre at standard temperature and pressure (0°C and 101.3 kPa)
AT	Ambient Temperature
calm	Wind conditions where the wind speed is below the operating range of the wind sensor
СО	Carbon monoxide
mm	Millimeters
NO	Nitric oxide
NO ₂	Nitrogen dioxide
NO _x	Oxides of nitrogen
PM ₁₀	Particulate less than 10 microns in equivalent aerodynamic diameter
PM _{2.5}	Particulate less than 2.5 microns in equivalent aerodynamic diameter
ppb	Parts per billion

NorthConnex



ppm	Parts per million
PPIII	i al to per minori

WD Vector Wind Direction

WS Vector Wind Speed

NorthConnex



Appendix 2 - Explanation of Exception Table

Automatic background check refers to when analyser samples zero air and measures the level of the concentration voltage. This voltage is taken as the zero-signal level and this value is subtracted from any subsequent readings as an active zero compensation. This is the analyser's fine zero measurement.

Beta count failure refers to a fault in the functioning of the EBAM. A one-minute beta count was less than the maximum acceptable counts during operation.

Calibration check outside tolerance refers to when the calibration values are outside the tolerance limits set for the precision check.

Calibration correction factor applied to data refers to an offset or multiplier applied to the data. This operation may be performed for a number of reasons including: (a) when a clear trend / drift outside the tolerance limit can be demonstrated by repeated operation precision checks, (b) when a correction is required on previously logged data due to a calibration check being outside the allowable tolerance

Commissioning refers to the initial setup and calibration of the instrument when it is first installed. For some instruments there may be a stabilisation period before normal operation commences.

Data transmission error refers to a period of time when the instrument could not transmit data. This may be due to interference, or a problem with the phone line or modem.

Equipment malfunction/instrument fault refers to a period of time when the instrument was not in the normal operating mode and did not measure a representative value of the existing conditions.

Gap in data/data not available refers to a period of time when either data has been lost or could not be collected.

Instrument Alarm refers to an alarm produced by the instrument. A range of alarms can be produced depending on how operation of the instrument is being affected.

Instrument out of service refers to a lack of data due to an instrument being shut down for repair, maintenance, or factory calibration.

Linear offset or multiplier refers to when an offset or multiplier has been applied between two points where the values of the offset or multiplier are different and the correction is interpolated between the two points.

NorthConnex

Report No: DAT15689





Logger error refers to when an error occurs and instrument readings are not correctly recorded by the logger.

Maintenance refers to a period of time when the logger/instrument was switched off due to maintenance.

Overnight span/zero out of tolerance refers to when the span/zero reading measured by the analyser during an automatic precision check falls outside of the expected concentration limits.

Power Interruption refers to no power to the station therefore no data was collected at this time.

Remote Calibration refers to when a technician remotely connects to the station and manually performs a span check.

Stabilisation after power interruption refers to the startup period of an instrument after power has been restored.

Static offset or multiplier refers to when a single offset or multiplier has been applied to the data between two points either to increase or decrease the measured value.

Tape break refers to the breaking of the EBAM/BAM sample tape during operation.